



# SARS-COV-2 VIRUS (COVID-19) IgG/IgM Rapid Test Cassette

(WB/S/P)

English



For professional and in vitro diagnostic use only.

## [INTENDED USE]

The SARS-COV-2 VIRUS (COVID-19) IgG/IgM Rapid Test Cassette is a lateral flow chromatographic immunoassay for the qualitative detection of antibodies (IgG and IgM) to SARS-CoV-2 in human Whole Blood/Serum/Plasma. The test is intended to be used at clinical laboratories or by healthcare workers, not for home use. This test has not been reviewed by the FDA. Negative results do not rule out SARS-CoV-2 infection, particularly in those who have been in contact with the virus. Follow-up testing with a molecular diagnostic should be considered to rule out infection in these individuals. Results from antibody testing should not be used as the sole basis to diagnose or exclude SARS-CoV-2 infection or to inform infection status. Positive results may be due to past or present infection with non-SARS-CoV-2 coronavirus strains, such as coronavirus HKU1, NL63, OC43, or 229E. Not for the screening of donated blood.

## [SUMMARY]

Early January 2020, a novel coronavirus (SARS-CoV-2, formerly known as 2019-nCoV) was identified as the infectious agent causing an outbreak of viral pneumonia in Wuhan, China, where the first cases had their symptom onset in December 2019.

Coronaviruses are enveloped RNA viruses that are distributed broadly among humans, other mammals, and birds and that cause respiratory, enteric, hepatic, and neurological diseases. Six coronavirus species are known to cause human disease. Four viruses-229E, OC43, NL63, and HKU1 are prevalent and typically cause common cold symptoms in immunocompetent individuals. The two other strains severe acute respiratory syndrome coronavirus (SARS-CoV) and Middle East respiratory syndrome coronavirus (MERS-CoV) are zoonotic in origin and have been linked to sometimes fatal illness.

Coronaviruses are zoonotic, meaning they are transmitted between animals and people. Common signs of infection include respiratory symptoms, fever, cough, shortness of breath and breathing difficulties. In more severe cases, infection can cause pneumonia, severe acute respiratory syndrome, kidney failure and even death.

Standard recommendations to prevent infection spread include regular hand washing, covering mouth and nose when coughing and sneezing, thoroughly cooking meat and eggs. Avoid close contact with anyone showing symptoms of respiratory illness such as coughing and sneezing.

## [PRINCIPLE]

The SARS-COV-2 VIRUS (COVID-19) IgG/IgM Rapid Test Cassette is a qualitative membrane strip based immunoassay for the detection of antibodies (IgG and IgM) to SARS-CoV-2 in human Whole Blood/Serum/Plasma. The test cassette consists of: 1) a burgundy colored conjugate pad containing SARS-CoV-2 Virus recombinant envelope antigens conjugated with Colloid gold (SARS-CoV-2 conjugates), 2) a nitrocellulose membrane strip containing two test lines (IgG and IgM lines) and a control line (C line). The IgM line is pre-coated with the Mouse anti-Human IgM antibody, IgG line is coated with Mouse anti-Human IgG antibody. When an adequate volume of test specimen is dispensed into the sample well of the test cassette, the specimen migrates by capillary action across the cassette. IgM anti-SARS-CoV-2, if present in the specimen, will bind to the SARS-CoV-2 conjugates. The immunocomplex is then captured

by the reagent pre-coated on the IgM band, forming a burgundy colored IgM line, indicating a SARS-CoV-2 IgM positive test result. IgG anti-SARS-CoV-2 if present in the specimen will bind to the SARS-CoV-2 conjugates. The immunocomplex is then captured by the reagent coated on the IgG line, forming a burgundy colored IgG line, indicating a SARS-CoV-2 IgG positive test result. Absence of any T lines (IgG and IgM) suggests a negative result. To serve as a procedural control, a colored line will always appear at the control line region indicating that proper volume of specimen has been added and membrane wicking has occurred.

## [WARNINGS AND PRECAUTIONS]

- For in vitro diagnostic use only.
- For healthcare professionals and professionals.
- Do not use after the expiration date.
- Please read all the information in this leaflet before performing the test.
- The test cassette should remain in the sealed pouch until use.
- All specimens should be considered potentially hazardous and handled in the same manner as an infectious agent.
- The used test cassette should be discarded according to federal, state and local regulations.

## [COMPOSITION]

The test contains a membrane strip coated with Mouse anti-Human IgM antibody and Mouse anti-Human IgG antibody on the test line, and a dye pad which contains colloidal gold coupled with SARS-CoV-2 recombinant antigen.

The quantity of tests was printed on the labeling.

### Materials Provided

- Test cassette
- Buffer
- Package insert

### Materials Required But Not Provided

- Specimen collection container
- Timer

## [STORAGE AND STABILITY]

- Store as packaged in the sealed pouch at the temperature (4-30°C or 40-86°F). The kit is stable within the expiration date printed on the labeling.
- Once open the pouch, the test should be used within one hour. Prolonged exposure to hot and humid environment will cause product deterioration.
- The LOT and the expiration date were printed on the labeling.


## [SPECIMEN]

- The test can be used to test Whole Blood/Serum/Plasma specimens.
- To collect whole blood, serum or plasma specimens following regular clinical laboratory procedures.
- Separate serum or plasma from blood as soon as possible to avoid hemolysis. Use only clear non-hemolyzed specimens.
- Store specimens at 2-8°C (36-46°F) if not tested immediately. Store specimens at 2-8°C up to 7 days. The specimens should be frozen at -20°C (-4°F) for longer storage. Do not freeze whole blood specimens.
- Avoid multiple freeze-thaw cycles. Prior to testing, bring frozen specimens to room temperature slowly and mix gently. Specimens containing visible particulate matter should be clarified by centrifugation before testing.
- Do not use samples demonstrating gross lipemia, gross hemolysis or turbidity in order to avoid interference on result interpretation.

## [TEST PROCEDURE]

Allow the test device and specimens to equilibrate to temperature (15-30°C or 59-86°F) prior to testing.

1. Remove the test cassette from the sealed pouch.
2. Hold the dropper vertically and transfer 1 drop of specimen (approximately 10µl) to the specimen well(S) of the test device, then add 2 drops of buffer (approximately 70µl) and start the timer. See the illustration below.
3. Wait for colored lines to appear. Interpret the test results in 15 minutes. Do not read results after 20 minutes.

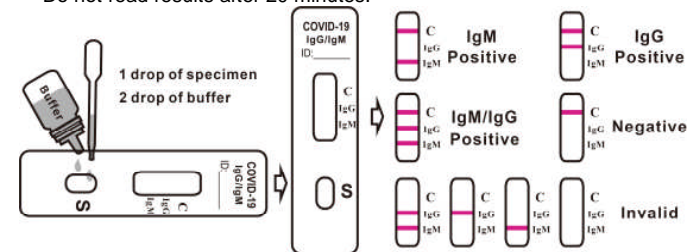

(The picture is for reference only, please refer to the material object.)

## [INTERPRETATION OF RESULTS]

**Positive:** Control line and at least one test line appear on the membrane. The appearance of IgG test line indicates the presence of SARS-CoV-2 specific IgG antibodies. The appearance of IgM test line indicates the presence of SARS-CoV-2 specific IgM antibodies. And if both IgG and IgM line appear, it indicates that the presence of both SARS-CoV-2 specific IgG and IgM antibodies.

**Negative:** One colored line appears in the control region (C). No apparent colored line appears in the test line region.

**Invalid:** Control line fails to appear. Insufficient specimen volume or incorrect procedural techniques are the most likely reasons for control line failure. Review the procedure and repeat the test with a new test cassette. If the problem persists, discontinue using the test kit immediately and contact your local distributor.

## [QUALITY CONTROL]

A procedural control is included in the test. A colored line appearing in the control region (C) is considered an internal procedural control. It confirms sufficient specimen volume, adequate membrane wicking and correct procedural technique.

Control standards are not supplied with this kit. However, it is recommended that positive and negative controls be tested as good laboratory practice to confirm the test procedure and to verify proper test performance.

## [LIMITATIONS]

- The SARS-COV-2 VIRUS (COVID-19) IgG/IgM Rapid Test Cassette is limited to provide a qualitative detection. The intensity of the test line does not necessarily correlate to the concentration of the antibody in the blood.
- Each physician must interpret the results in conjunction with the patient's history, physical findings, and other diagnostic procedures.
- A negative test result indicates that antibodies to SARS-CoV-2 are either not present or at levels undetectable by the test.

## [PERFORMANCE CHARACTERISTICS]

### Accuracy

Summary data of SARS-COV-2 VIRUS (COVID-19) IgG/IgM Rapid Test as below:

Regarding the IgM test, the result comparison to RT-PCR.

**SARS-COV-2 VIRUS (COVID-19) IgM:**

SARS-COV-2 VIRUS (COVID-19) IgM	RT-PCR		Total
	Positive	Negative	
<b>CLUNGENE®</b> Positive	67	1	68
Negative	10	89	99
<b>Total</b>	<b>77</b>	<b>90</b>	<b>167</b>

A statistical comparison was made between the results yielding a sensitivity of 87.01%, a specificity of 98.89% and an accuracy of 93.41%

Regarding the IgG test, we have counted the positive rate of the 77 patients during the convalescence period.

**SARS-COV-2 VIRUS (COVID-19) IgG:**

SARS-COV-2 VIRUS (COVID-19) IgG	Number of patients during the convalescence period	Total
<b>CLUNGENE®</b> Positive	75	75
Negative	2	2
<b>Total</b>	<b>77</b>	<b>77</b>

**Class Specificity**

Both SARS-CoV-2(COVID-19) IgM and IgG negative specimen were tested. The IgM line is specific to IgM( not falsely detecting IgG) and IgG is specific for IgG(not falsely detecting IgM).It indicates that class specificity is good in these tests.

**Cross-Reactivity and Interference**

- Other common causative agents of infectious diseases were evaluated for cross reactivity with the test. Some positive specimens of other common infectious diseases were spiked into the SARS-CoV-2 positive and negative specimens and tested separately. No cross reactivity was observed with specimens from patients infected with HIV, HAV, HBsAg, HCV, TP, HTLV, CMV, FLUA, FLUB, RSV, MP, CP, HPIVs.
- Potentially cross-reactive endogenous substances including common serum components, such as lipids, hemoglobin, bilirubin, were spiked at high concentrations into the SARS-CoV-2 positive and negative specimens and tested, separately. No cross reactivity or interference was observed to the device.

Analytes	Conc.	Specimens	
		Positive	Negative
Albumin	20mg/ml	+	-
Bilirubin	20µg/ml	+	-
Hemoglobin	15mg/ml	+	-
Glucose	20mg/ml	+	-
Uric Acid	200µg/ml	+	-
Lipids	20mg/ml	+	-

- Some other common biological analytes were spiked into the SARS-CoV-2 positive and negative specimens and tested separately. No significant interference was observed at the levels listed in the table below.

Analytes	Conc. (µg/ml)	Specimens	
		Positive	Negative
Acetaminophen	200	+	-
Acetoacetic Acid	200	+	-
Acetylsalicylic Acid	200	+	-
Benzoylcegonine	100	+	-

Caffeine	200	+	-
EDTA	800	+	-
Ethanol	1.0%	+	-
Gentisic Acid	200	+	-
β - Hydroxybutyrate	20,000	+	-
Methanol	10.0%	+	-
Phenothiazine	200	+	-
Phenylpropanolamine	200	+	-
Salicylic Acid	200	+	-

**Reproducibility**

Reproducibility studies were performed for SARS-CoV-2 Virus IgG/IgM Rapid Test at three physician office laboratories (POL). Sixty (60) clinical serum specimens, 20 negative, 20 borderline positive and 20 positive, were used in this study. Each specimen was run in triplicate for three days at each POL. The intra-assay agreements were 100%. The inter-site agreement was 100%.

**[ DISCLAIMER NOTICE ]**

- This test has not been reviewed by the FDA.
- Negative results do not rule out SARS-CoV-2 infection, particularly in those who have been in contact with the virus. Follow-up testing with a molecular diagnostic should be considered to rule out infection in these individuals.
- Results from antibody testing should not be used as the sole basis to diagnose or exclude SARS-CoV-2 infection or to inform infection status.
- Positive results may be due to past or present infection with non-SARS-CoV-2 coronavirus strains, such as coronavirus HKU1, NL63, OC43, or 229E.



Hangzhou Clongene Biotech Co., Ltd.  
No.1 Yichuang Road, Yuhang Sub-district, Yuhang District,  
311121 Hangzhou, China

**EC REP** Shanghai International Holding Corp.GmbH (Europe)  
Eiffestrasse 80, D-20537 Hamburg, Germany

**Index of Symbol**

Do not reuse For in vitro diagnostic use only

Store between 4-30°C  
 Caution  
 Use by  
 Keep away from sunlight  
 Manufacturer  
 Consult instructions for use  
 Lot number  
 Contains sufficient for <n> tests  
 Keep dry  
 Do not use if package is damaged  
**EC REP** Authorized representative in the European Community

Version No.: 2.0  
Effective Date: Mar. 27, 2020